



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

AlpaSuri GbR/Barbara Bruns & Wolfgang Stamp
Elbuferstr. 12
21423 Winsen/Luhe Germany

07/29/19

Test No: 977024


Animal and Sample Description

Animal Name: Dance Away
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 953010002470746
Sample Location: Mid Side
Sample Date: 04/28/19
Age: 12/11/13

Laboratory Data

Mean Fiber Diameter:	18.4 microns	Spin Fineness:	17.7 microns
Standard Deviation:	3.6 microns	Mean Curvature (deg/mm):	60.2
Coefficient of Variation:	19.7 %	SD Curvature (deg/mm):	29.9
Fibers Greater Than 30 microns:	0.6 %	Comfort Factor:	99.4 %
Medullated Fibers:	5.7 %		

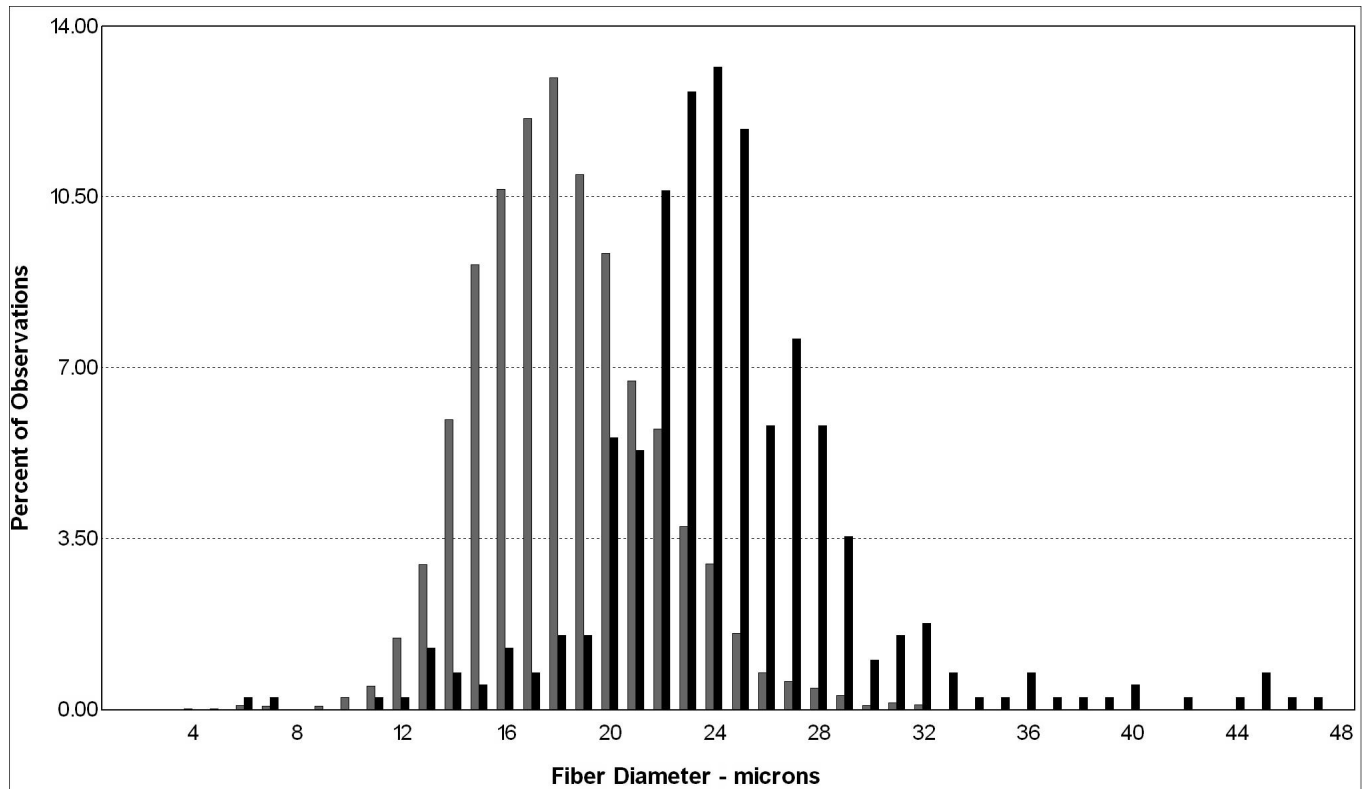

This Test Performed According to I.W.T.O Method 47