



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

AlpaSuri GbR/Barbara Bruns & Wolfgang Stamp
Elbuferstr. 12
21423 Winsen/Luhe Germany

07/29/19

Test No: 977030


Animal and Sample Description

Animal Name: Frieda
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 000771D373
Sample Location: Mid Side
Sample Date: 04/28/19
Age: 01/15/14

Laboratory Data

Mean Fiber Diameter:	21.0 microns	Spin Fineness:	20.3 microns
Standard Deviation:	4.2 microns	Mean Curvature (deg/mm):	46.4
Coefficient of Variation:	20.1 %	SD Curvature (deg/mm):	26.1
Fibers Greater Than 30 microns:	3.2 %	Comfort Factor:	96.8 %
Medullated Fibers:	7.3 %		

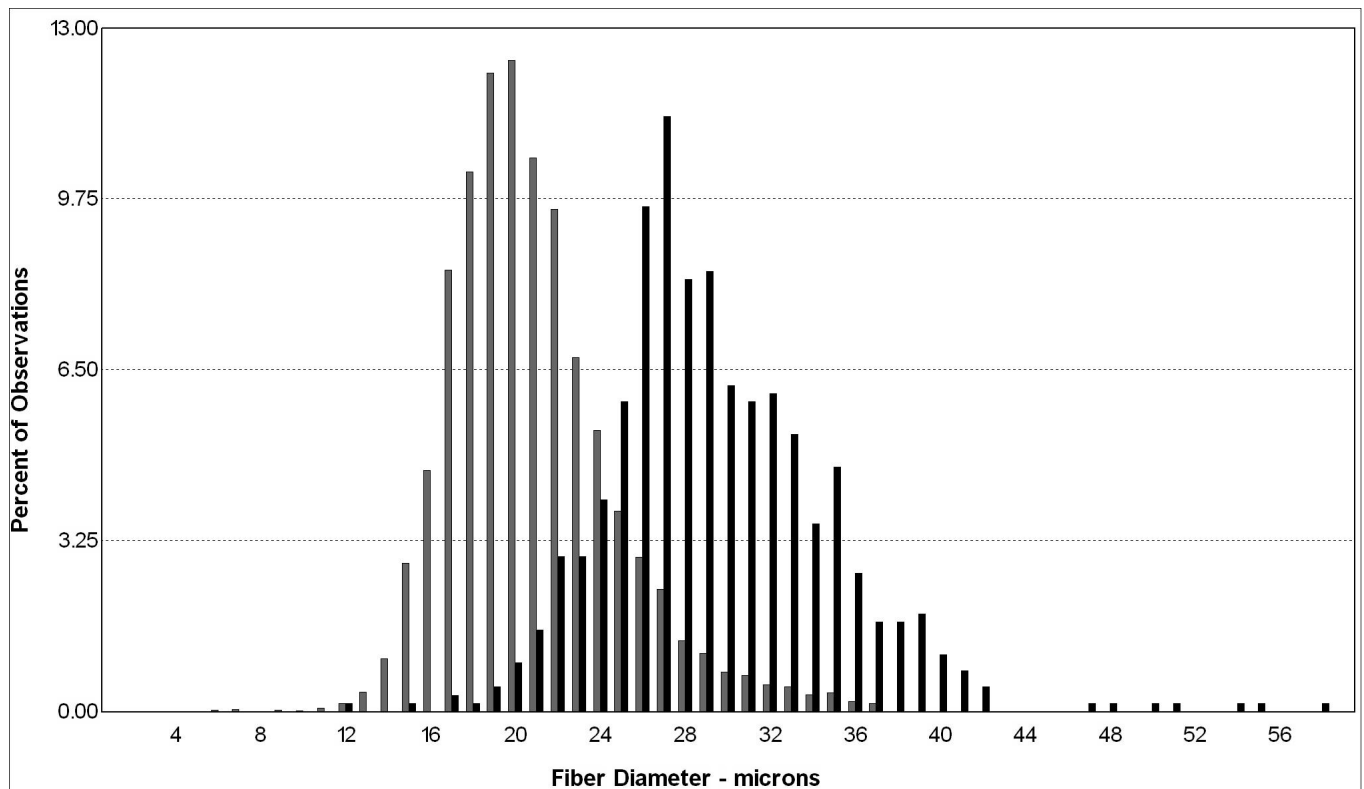

This Test Performed According to I.W.T.O Method 47