



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

AlpaSuri GbR/Barbara Bruns & Wolfgang Stamp
Elbuferstr. 12
21423 Winsen/Luhe Germany

07/29/19

Test No: 977033


Animal and Sample Description

Animal Name: Giselle
Breed: Alpaca(Suri)
Sex: Female
Color: White

Animal ID: 953010001046594
Sample Location: Mid Side
Sample Date: 04/28/19
Age: 02/14/14

Laboratory Data

| | | | |
|--|--------------|---------------------------------|--------------|
| Mean Fiber Diameter: | 18.1 microns | Spin Fineness: | 17.3 microns |
| Standard Deviation: | 3.5 microns | Mean Curvature (deg/mm): | 16.9 |
| Coefficient of Variation: | 19.4 % | SD Curvature (deg/mm): | 20.3 |
| Fibers Greater Than 30 microns: | 0.7 % | Comfort Factor: | 99.3 % |
| Medullated Fibers: | 0.4 % | | |

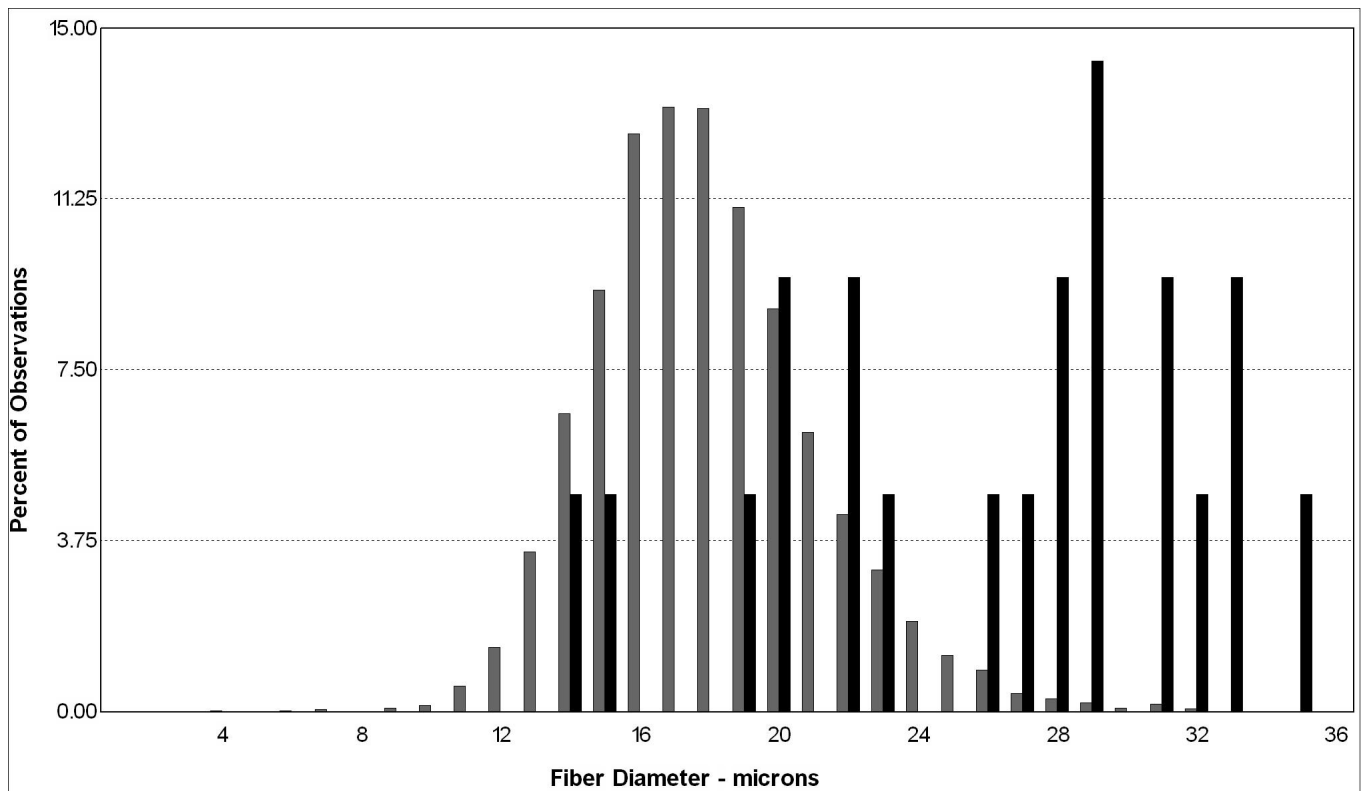

This Test Performed According to I.W.T.O Method 47