

Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

AlpaSuri GbR/Barbara Bruns & Wolfgang Stamp
Elbuferstr. 12
21423 Winsen/Luhe Germany

07/29/19

Test No: 977042


Animal and Sample Description

Animal Name: Jailli
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 000771B131
Sample Location: Mid Side
Sample Date: 04/28/19
Age: 11/15/13

Laboratory Data

Mean Fiber Diameter:	23.2 microns	Spin Fineness:	21.9 microns
Standard Deviation:	4.0 microns	Mean Curvature (deg/mm):	43.9
Coefficient of Variation:	17.3 %	SD Curvature (deg/mm):	23.6
Fibers Greater Than 30 microns:	3.9 %	Comfort Factor:	96.1 %
Medullated Fibers:	12.4 %		

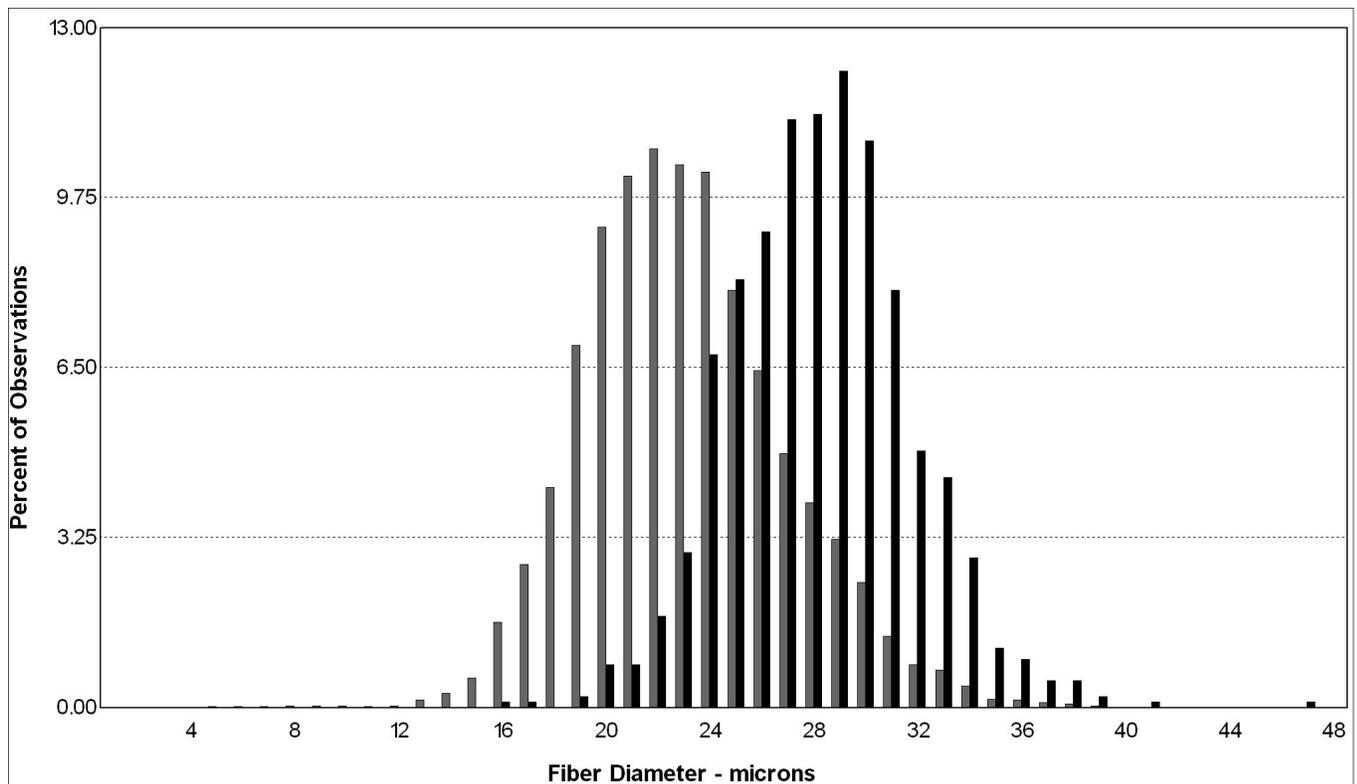

This Test Performed According to I.W.T.O Method 47