



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

AlpaSuri GbR/Barbara Bruns & Wolfgang Stamp
Elbuferstr. 12
21423 Winsen/Luhe Germany

07/29/19

Test No: 977063


Animal and Sample Description

Animal Name: Qilla
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 00070ABBD8
Sample Location: Mid Side
Sample Date: 04/28/19
Age: 05/15/13

Laboratory Data

Mean Fiber Diameter:	19.3 microns	Spin Fineness:	18.3 microns
Standard Deviation:	3.4 microns	Mean Curvature (deg/mm):	53.7
Coefficient of Variation:	17.8 %	SD Curvature (deg/mm):	27.4
Fibers Greater Than 30 microns:	0.9 %	Comfort Factor:	99.1 %
Medullated Fibers:	1.9 %		

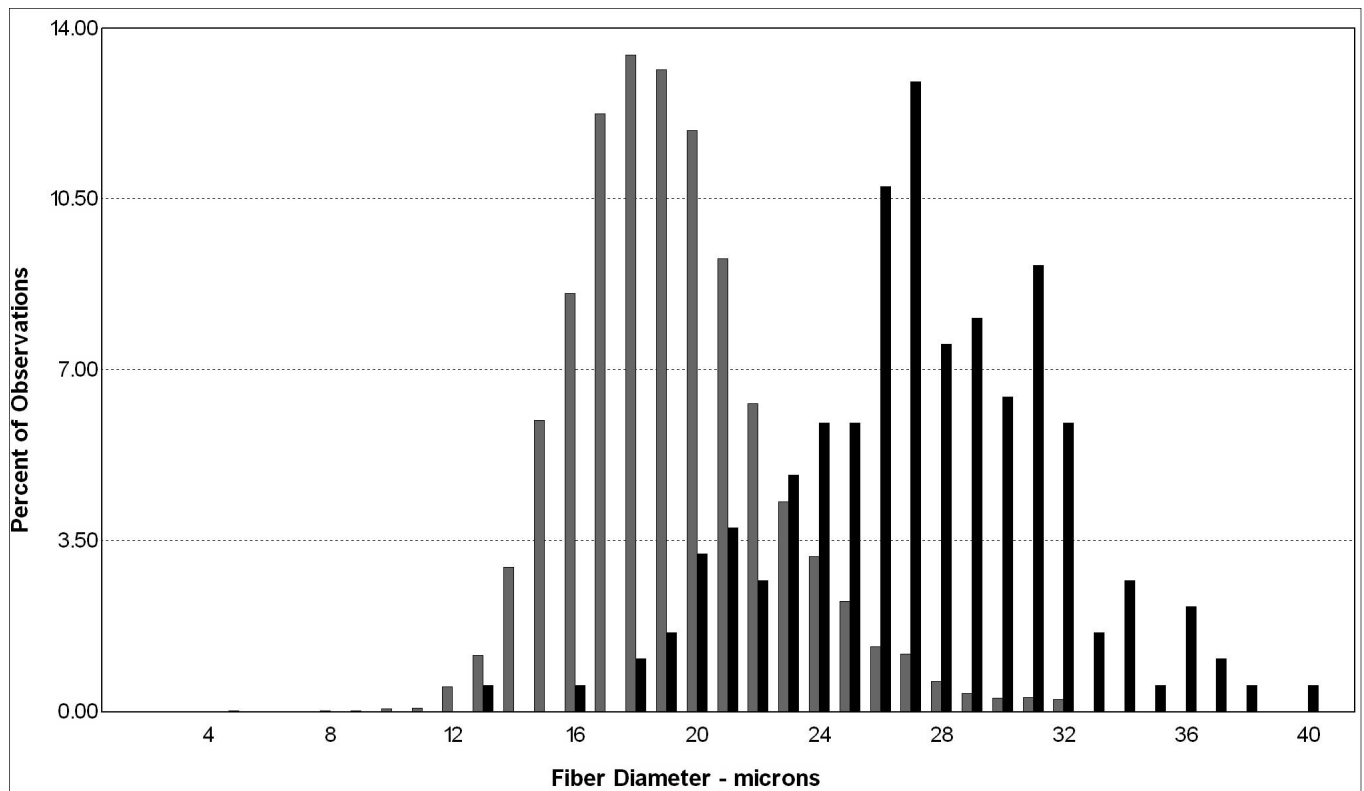

This Test Performed According to I.W.T.O Method 47