



Yocom-McColl Testing Laboratories, Inc.

540 West Elk Place • Denver, Colorado 80216-1823 USA

PHONE (303) 294-0582 • FAX (303) 295-6944

EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA100) Micron Test Report

AlpaSuri GbR/Barbara Bruns & Wolfgang Stamp
Elbuferstr. 12
21423 Winsen/Luhe Germany

07/29/19

Test No: 977091


Animal and Sample Description

Animal Name: Warakusi
Breed: Alpaca(Huacaya)
Sex: Female
Color: White

Animal ID: 00070A9DE4
Sample Location: Mid Side
Sample Date: 04/28/19
Age: 11/15/12

Laboratory Data

Mean Fiber Diameter:	17.2 microns	Spin Fineness:	16.9 microns
Standard Deviation:	3.8 microns	Mean Curvature (deg/mm):	59.8
Coefficient of Variation:	22.2 %	SD Curvature (deg/mm):	31.5
Fibers Greater Than 30 microns:	0.5 %	Comfort Factor:	99.5 %
Medullated Fibers:	3.6 %		

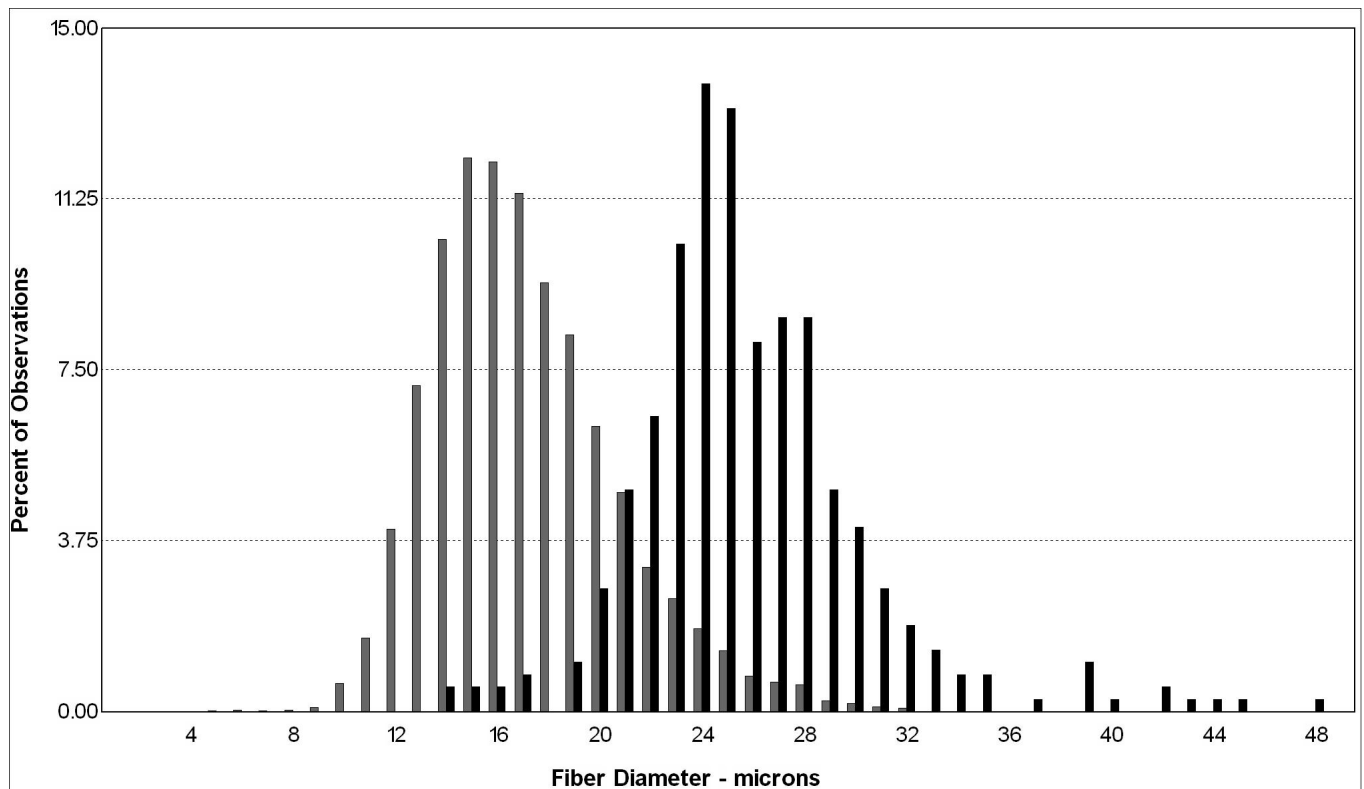

This Test Performed According to I.W.T.O Method 47